

**User's Manual**  
**for**  
**WavePond® DAx11500z-LAN, DAx11000z-LAN**  
**Arbitrary WaveForm Generators**

**1-Channel, 1.5 GS/sec, 9-bit** (DAx11500z-LAN)

**1-Channel, 1.0 GS/sec, 9-bit** (DAx11000z-LAN)

**Chase Scientific LLC**

P.O. Box 1487  
Langley, WA 98260

Web: <https://chase-scientific.com/wavepond.html>

Original Document: dax11500z\_lan\_manual.odt

(created 04/06/24, updated 05/06/24)

**© 2024 by WavePond®, division of Chase Scientific LLC**

This manual, the DAx11500z-LAN, DAx11000z-LAN modules, and the software outlined in this document are copyrighted with all rights reserved. Under the copyright laws, the above mentioned may not be copied, in whole or in part, without the express written consent of Chase Scientific LLC. WavePond® is a registered trademark of Chase Scientific LLC.

## TABLE OF CONTENTS

---

<b>1 GENERAL INFORMATION.....</b>	<b>3</b>
1.1 INTRODUCTION.....	3
1.2 REFERENCES.....	3
1.3 DELIVERABLES.....	4
1.3.1 Software.....	4
1.3.2 Hardware.....	4
1.3.3 DAX11500z Checklist.....	5
1.4 PRODUCT SPECIFICATION.....	5
1.5 TECHNICAL SUPPORT / SOFTWARE UPDATES.....	6
1.6 FCC WARNING.....	6
1.7 WARRANTY.....	6
<b>2 QUICK START GUIDE FOR WAVEPOND DAX11500Z-LAN (WINDOWS 10/11).....</b>	<b>7</b>
<b>3 SCRIPT EDITOR (COMMAND.TXT GENERATOR).....</b>	<b>9</b>
3.1 INTRODUCTION.....	9
3.2 OPERATION.....	9
<b>4 COMMAND DESCRIPTIONS / USAGE.....</b>	<b>10</b>
4.0.1 Typical "command.txt" file.....	10
4.0.2 Complete Command Descriptions / Usage.....	10
4.0.2.1 init.....	10
4.0.2.2 set_clock <value_Hz_Float>.....	10
4.0.2.3 load_wfm <data_file / level / loop / trigger>.....	10
4.0.2.4 run.....	11
4.0.2.5 stop.....	11
4.0.3 set_rtz <rtz_mode>.....	11
4.0.4 set_mux (internal use only).....	12
<b>5 MISCELLANEOUS.....</b>	<b>13</b>
5.1 CALIBRATION.....	13
5.2 MAINTENANCE.....	13

## ILLUSTRATIONS / TABLES

## **1 GENERAL INFORMATION**

---

### **1.1 Introduction**

{  
*For **BREVITY** for the rest of this document both the **DAX11500z-LAN** and the **DAX11000z-LAN** will be referred to as **DAX11500** unless specific data requires a distinction between the two such as specifications.*  
}

The DAX11500z-LAN and DAX11000z-LAN are LAN based Arbitrary Waveform Generators with a maximum sampling rate of 1.5 GS/sec and 1.0 GS/sec respectively. They are designed to produce any waveform from DC up to and even past many times Nyquist frequency using bands and/or using RTZ mode. The 9-bit D/A and on-board high resolution frequency synthesizer allow the user to seamlessly fit looping waveforms into memory, alleviating the need for more expensive and less reliable options.

#### **The DAX11500 module has the following standard features:**

- (1) Channel, 1.5 GS/sec, 9-bit D/A outputs (750 mVpp Typical) [SMA]
- DC Coupled outputs into 50 ohms
- 1ppm Internal Programmable Clock Synthesizer with < 5psec Jitter (typical)
- Internal Clock Synthesizer operates from 25 MHz to 1.5 GHz. (1.0 GHz for DAX11000)
- SFDR less than -40 dB @ 500 MHz (typ)
- Full scale Trise/Tfall = 150 picoseconds (typical)
- 8000 Samples Memory
- 3.3V TTL Prog. Marker Out [SMA]
- 3.3V TTL TRIG\_IN (Asynchronous Trigger Capability with 667 psec resolution) [SMA]
- Ethernet box powered by 12V DC power brick.
- All functions controlled through network share over Ethernet via text files.

### **1.2 References**

See LAN specifications for GBit Ethernet applications. The DAX11500z-LAN requires a local area network with a DHCP service and user PC connected to same.

## 1.3 Deliverables

### 1.3.1 Software

Since the DAX11500z-LAN is controlled when a text file called "command.txt" is copied to the DAX11500 file share, it doesn't need any traditional software drivers or API. For convenience, and to expedite initial debug, we have provided a program called "run\_script.exe". This program allows you to edit the text commands, save, and create a copy called "command.txt" on the file share called "\\raspberrypi\Ramdisk\_Share". However, you will need to copy your waveform files to the DAX11500 file share separately.

Please note that the "command.txt" file must be padded with blank lines to guarantee it has 30 or more total lines in the text file.

**TBD:**

*GUI program (dax115\_lan.exe) can perform many tasks including loading waveforms from a file, generating sine, square, triangle, and sawtooth waves, changing clock rates, triggering etc.*

### 1.3.2 Hardware

By default the DAX11500z hardware consists of an aluminum box, Ethernet connector, and 12V power brick. The customer must provide the Ethernet cable.



### 1.3.3 DAX11500z Checklist

Item #	Qty	Part Number	Description
1	1	DAX11500z-LAN	(1) Channel, 1.5 GSPS, 9-bit, Arbitrary Waveform Generator System housed in Ethernet controlled aluminum box with 8K Memory.

## 1.4 Product Specification

**DAX11500** (all specifications are at 25C unless otherwise specified)

### I/O SPECIFICATIONS

<b>Analog Outputs (SMA)</b>	
Number of D/A Outputs	1
Vertical Resolution	9-bits
Output Impedance	50 ohms
Amplitude	750 mVpp typical into 50 ohms
T(rise) / T(fall)	150 psec typical
Memory Size	8K samples
Maximum # of Segments	1
Segment Size Range	16 samples up to total memory; Modulo 4 only.
Segment Resolution	4 samples
Maximum Segment Loops	1, infinite
<b>LVTTL Outputs (SMA)</b>	(1) Marker Outputs (3.3V TTL). One at beginning of waveform and one user programmable.
<b>LVTTL Inputs (SMA)</b>	(1) Trigger input (3.3V). Input is DC coupled to 0.9V into 50 ohms. Actual trigger level is 1.0V. Trigger delay = TBD.  See software function description for functionality. Maximum re-trigger rate is approximately 500 KHz.
<b>Master Clock (internal)</b>	
Frequency	25 MHz to 1.5 GHz standard
Phase Noise	-100dBc/Hz @ 1KHz Offset Typical @ Fc = 1.5 GHz
Jitter	< 5 picoseconds

### GENERAL

Power Supply (Vcc)	+ 12.0V +/- 10%, 2A typical.
Operating Temperature	15 to 30 degrees C standard
Operating Humidity	5 to 95% non-condensing
Size	6" x 6.5" x 2.5"
Data Bus	Ethernet

## 1.5 Technical Support / Software Updates

For technical support:

Sales/Tech	<a href="https://chase-scientific.com/sales.html">https://chase-scientific.com/sales.html</a>
Mail	Chase Scientific P.O. Box 1487 Langley, WA 98260
Software	<a href="https://chase-scientific.com/wavepond.html.com">https://chase-scientific.com/wavepond.html.com</a>

## 1.6 FCC Warning

This equipment is intended for use in a laboratory test environment only. The equipment generates, uses, and can radiate radio frequency energy and has not been tested for compliance with the limits of computing devices pursuant to subpart J of part 15 of FCC rules, which are designed to provide reasonable protection against radio frequency interference. Operation of this equipment in other environments may cause interference with radio communications, in which case, the user, at their own expense, is required to take whatever measures may be required to correct this interference.

## 1.7 Warranty

WavePond warrants to the original purchaser that its DAX11500z-LAN, DAX11000z-LAN, and the component parts thereof, will be free from defects in workmanship and materials for a period of ONE YEAR from the date of purchase.

WavePond will, without charge, repair or replace at its option, defective or component parts upon delivery to WavePond's service department within the warranty period accompanied by proof of purchase date in the form of a sales receipt.

**EXCLUSIONS:** This warranty does not apply in the event of misuse or abuse of the product or as a result of unauthorized alterations or repairs. It is void if the serial number is altered, defaced or removed.

WavePond shall not be liable for any consequential damages, including without limitation damages resulting from loss of use. Some states do not allow limitation or incidental or consequential damages, so the above limitation or exclusion may not apply to you.

This warranty gives you specific rights. You may also have other rights that vary from state to state.

WavePond warrants products "directly" sold anywhere in the world. If a WavePond product is purchased through an authorized distributor then warranty details are resolved through them.

**NOTICE:** WavePond reserves the right to make changes and/or improvements in the product(s) described in this manual at any time without notice.

---

**2 Quick Start Guide for WavePond DAX11500z-LAN (Windows 10/11)**

---

**Quick Start Guide for WavePond DAX11500z-LAN (Windows 10/11)**

**1)** Connect the included 12V Power Brick to the DAX11500. Then connect your local area network (LAN) Ethernet cable to the DAX11500. This network should include the computer you're planning on using to control the DAX11500.

-----

**2)** Turn on the DAX11500's power switch. The PWR light will blink for 25 seconds while the onboard computer is booting up. During boot-up the DAX11500 will obtain a local IP address from your DHCP server that manages your local area network.

-----

**3)** After DAX11500 has booted up it will create a network shared folder that is described as follows:

**\\raspberrypi\Ramdisk\_Share** [case sensitive]

It can take your Windows machine anywhere from 2 to 20 seconds to find this share. After allowing for this time you should be able to copy files to this share. However, for better usability we recommend assigning a drive letter to this share using the command line **terminal** like the following:

**net use w: \\raspberrypi\Ramdisk\_Share**

You can now open the share using File Manager (or click This PC on desktop). For initial testing purposes you can drag-and-drop all the data waveform files onto **drive w:** so you won't have to copy them later. The DAX11500 only uses local waveform files located in this share.

-----

**4)** Go to "[https://chase-scientific.com/dax11500z\\_lan.html](https://chase-scientific.com/dax11500z_lan.html)" and download "**dax11500z-lan.zip**" which includes this quick-start guide, manual, and "**run\_script.exe**". In near future there will be a Exerciser GUI for click button testing similar to the USB version.

-----

**Quick Start Guide for WavePond DAX11500z-LAN (Windows 10/11) cont.**

5) For quick verification run the program "run\_script.exe". Adjust parameters as needed. The unit boots up with the clock set to 1.5 GSamples/sec. Minimum commands are the following:

```
stop
load_wfm sweep2.txt 255 loop_1 trig_auto
run
```

Use "/" for comments. By clicking "Run Script" the program will copy what's on the screen to a file called "command.txt" to "\\raspberrypi\Ramdisk\_Share". Before it does that it pads the command.txt file with blank lines to insure that there are 31+ lines. (interpreter expects file to be 31 or more lines)

See manual for more details.

-----

**6) Recommended Settings to verify "command.txt" have completed (erased by DAX11500)**

Open PowerShell (run as Administrator) and execute the following commands:

```
Set-SmbClientConfiguration -DirectoryCacheLifetime 0
Set-SmbClientConfiguration -FileNotFoundCacheLifetime 0
Set-SmbClientConfiguration -FileInfoCacheLifetime 0
```

The default values for these are 10, 5, and 10 (seconds) respectively. These default values are extreme and prevent the network share's folder from showing that the "command.txt" file has been deleted in a timely fashion.

To see all the SMB client configuration information, including above, use the following:

```
Get-SmbClientConfiguration
```




### 3 Script Editor (command.txt generator)

#### 3.1 Introduction

This GUI application is provided to create and run script files.

#### 3.2 Operation

Below is a screen shot of "run\_script.exe". See next section for command descriptions. When "Run Script" button is pressed, anything on the screen is copied to a file called "command.txt" on the file share. The DAX11500 sees this and executes the file, then deletes the file. Please note that when this is done programmatically or manually, the file needs to be padded to at least 30 lines.

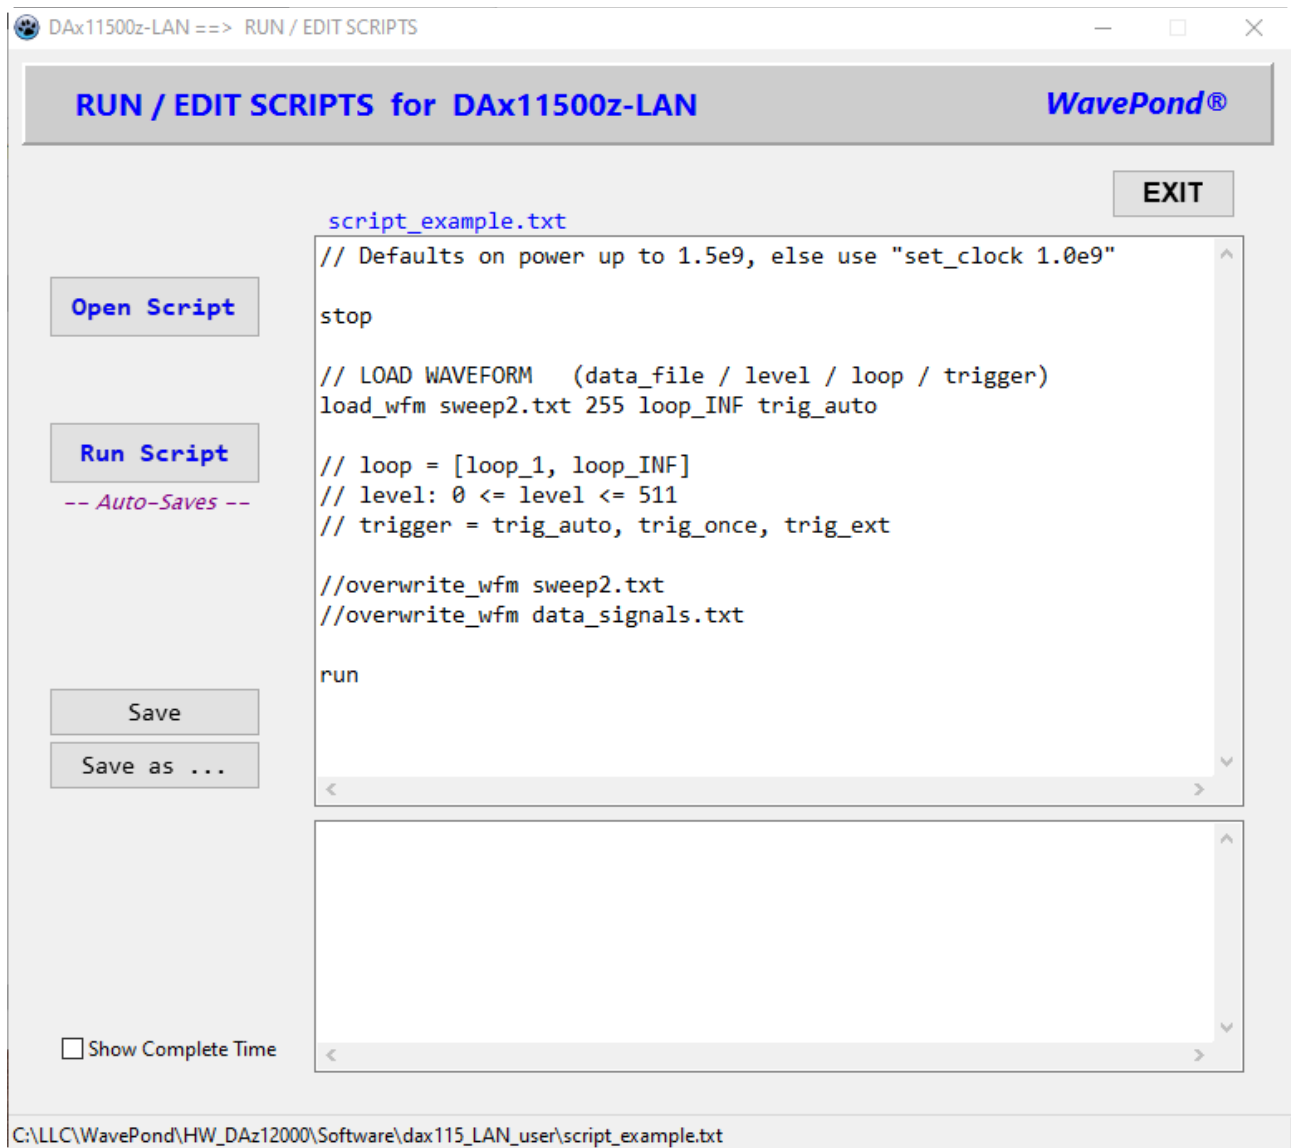

## 4 Command Descriptions / Usage

### 4.0.1 Typical "command.txt" file

```
// Defaults on power up to 1.5e9, else use "set_clock 1.0e9"
stop

// LOAD WAVEFORM (data_file / level / loop / trigger)
load_wfm sweep2.txt 255 loop_INF trig_auto

// loop = [loop_1, loop_INF]
// level: 0 <= level <= 511
// trigger = trig_auto, trig_once, trig_ext

run
```

### 4.0.2 Complete Command Descriptions / Usage

#### 4.0.2.1 init

##### Description

This command is called internally to the DAX11500 upon boot-up and should never need to be called again. Besides initializing variables it fills waveform memory with 255 (zero volts) and executes a run/stop cycle, leaving the output of the DAX11500 at zero volts.

##### Parameters

none

##### Example

init

#### 4.0.2.2 set\_clock <value\_Hz\_Float>

##### Description

Sets the Sampling Rate to the desired value in floating point format.

##### Parameters

value\_Hz\_Float: Must be between 25e6 and 1.5e9.

##### Example

```
set_clock 1.500e9      {sets sampling clock to 1.5 GHz}
```

#### 4.0.2.3 load\_wfm < data\_file / level / loop / trigger>

##### Description

Loads DA11500 with waveform "data\_file" with the parameters below. The stop command is typically used before this. However, if the size of the waveform file is the same, and the level, loop, and trigger is the same, THEN you can

simply substitute another "data\_file" ... it will update on-the-fly. Use "overwrite\_wfm" for even faster performance (ignores level, loop, and trigger ==> assumes they're the same).

### Parameters

level: 0 < level < 511 {this voltage shows up between triggered segments}  
loop = loop\_1 {one segment per trigger}  
loop\_inf {waveform is continuously looped (no gaps)}  
trig = trig\_auto {Internal Trigger every 1 msec}  
trig\_once {Internal Trigger occurs once}  
trig\_ext {External Trigger}

### Example

```
load_wfm 255 loop_1 trig_auto
```

## 4.0.2.4 run

### Description

Outputs the waveform previously setup.

### Parameters

none

### Example

```
dax115.exe run
```

## 4.0.2.5 stop

### Description

Stops waveform output.

### Parameters

none

### Example

```
dax115.exe stop
```

## 4.0.3 set\_rtz <rtz\_mode>

### Description

Stops waveform output.

### Parameters

rtz\_mode = 0 (deactivate)  
rtz\_mode = 1 (active - default)

### Example

`set_rtz 0` (turns off RTZ mode which is default)

#### **4.0.4 set\_mux (internal use only)**

## **5 MISCELLANEOUS**

---

### **5.1 Calibration**

The DAX11500 have no user features to perform calibration. DC offsets on the analog outputs can be adjusted by the factory to place the center value (255 out of 511) above, below, or at zero volts.

### **5.2 Maintenance**

No maintenance is required.

#### **Trademarks:**

WavePond is a registered trademark of Chase Scientific LLC. Windows is registered trademarks of Microsoft Corporation. macOS is a registered trademark of Apple Computer. Android is a registered trademark of Google.